

THE CHARACTERISTICS OF FAST SCINTILLATION DETECTORS OF TIME OF FLIGHT AND ANTICOINCIDENCE SYSTEM OF SPACE-BASED GAMMA-RAY TELESCOPE GAMMA-400 WITH SILICON PHOTOMULTIPLIERS READOUT

© 2022 A. I. Arkhangelskiy^{1*}, A. M. Galper^{1,2}, I. V. Arkhangelskaja¹, O. D. Dalkarov¹, M. G. Korotkov¹, A. A. Leonov^{1,2}, N. Yu. Pappe², S. I. Suchkov², N. P. Topchiev², M. D. Kheymits¹, E. N. Chasovikov¹, Yu. T. Yurkin¹

¹ National Research Nuclear University MEPhI (Moscow Engineering Physics Institute), Kashirskoe shosse 31, Moscow, 115409, Russia

² Lebedev Physical Institute, Russian Academy of Sciences, Leninskiy Prospekt 53, Moscow, 119991, Russia

* E-mail: aiarkhangelskij@mephi.ru

The main results obtained using ~250 MeV positron beam of synchrotron C-25P «PAKHRA» of P.N. Lebedev Physical Institute with prototype of time of flight and anticoincidence system of being developed space-based GAMMA-400 gamma-ray telescope are presented. The amplitude resolution, time resolution and charged particles detection efficiency are adduced. The comparison of using both «slow» and «fast» outputs of silicon photomultipliers of prototype scintillation detectors sensors is featured.

1. INTRODUCTION

The being developed scientific complex GAMMA-400 [1, 2] relates to the new generation of space observatories intended to perform an indirect search for signatures of dark matter in the cosmic-ray fluxes, precision investigation of characteristics of diffuse gamma-ray emission and gamma-rays from the Sun during periods of solar activity, gamma-ray bursts, extended and point gamma-ray sources in the wide energy range from several MeV up to TeV region, e^-/e^+ and cosmic-ray nuclei fluxes with energies up to $\sim 10^{15}$ eV by means of the GAMMA-400 gamma-ray telescope represents the core of the scientific complex. For gamma-rays with the energy >100 GeV the expected angular and energy resolution are $\sim 0.01^\circ$ and $\sim 2\%$ respectively and e^-/p rejection factor is $\sim 5 \cdot 10^5$ by preliminary estimations. The space observatory is planned for the launch at the end of this decade on the Navigator service platform [3] being designed by Lavochkin Association on the elliptical orbit with following initial parameters: an apogee ~ 300000 km, a perigee ~ 500 km, a rotation period ~ 7 days and inclination of 51.4° . At least 7 years of the active lifetime of the observatory is expected, reaching an unprecedented sensitivity in the indirect search of dark matter signatures and in the study of the unresolved and unidentified so

far gamma-ray sources. The planned scientific complex main technical parameters are: weight ~2500 kg, power consumption ~2000 W, total scientific and service downlink transmission up to 100 GByte/day.

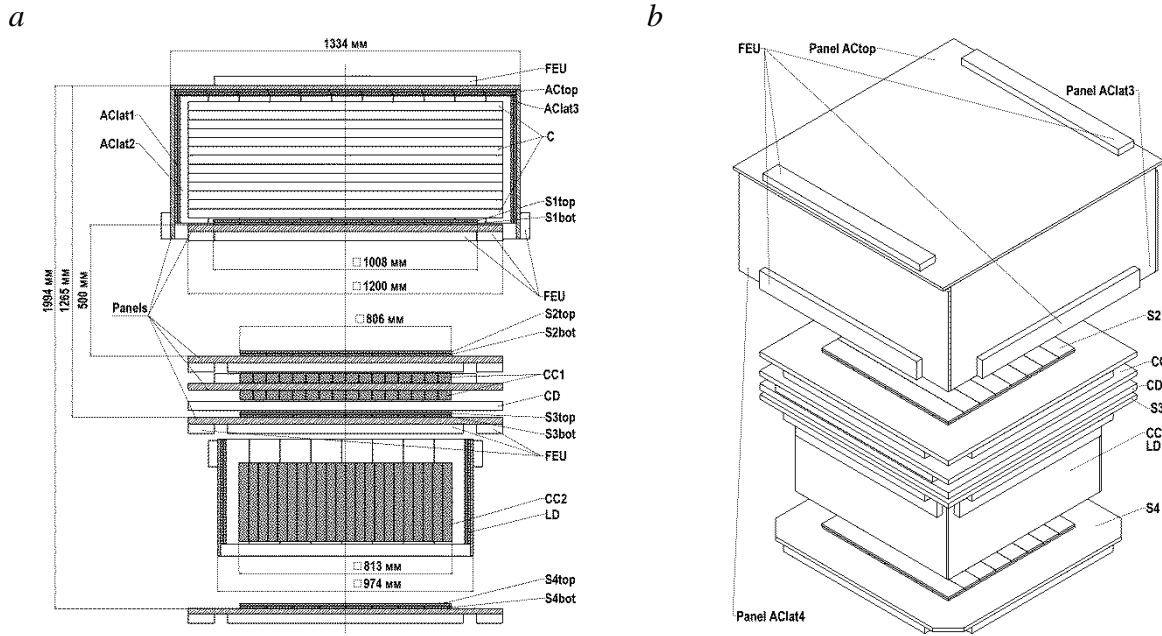


Fig. 1. The physical scheme of the GAMMA-400 gamma-ray telescope.

The physical scheme of under consideration variant of GAMMA-400 gamma-ray telescope is presented in Fig. 1. The converter-tracker C is used for high precision determination of the gamma-quanta conversion point and reconstruction of the trajectory of the primary and secondary charged particles. The converter-tracker consists of 13 layers of double (x, y) SciFi (0.25 mm scintillation fibers) tracking coordinates detectors with total thickness about $1X_0$ (X_0 - radiation length). The first 11 layers are interleaved with tungsten conversion foils (first 7 layers of $0.1X_0$ and next 4 layers of $0.025X_0$). The last two layers have no tungsten. The AC is segmented anticoincidence detector (135 scintillator strips) includes one top detector AC_{top} and four lateral detectors AC_{lat1} – AC_{lat4} surrounding convertor-tracker for discrimination between incoming charged particles and gamma-quanta with an efficiency of $\geq 99.95\%$. The LD is segmented anticoincidence detector (64 scintillator strips) includes four lateral detectors $LD1$ – $LD4$ surrounding total-absorption calorimeter CC2. All anticoincidence counters, as well as S3 and S4 are made of two oriented in parallel layers of 1 cm thickness, 10 cm width BC-408

polyvinyltoluene scintillator strips with different length. The strips of one layer are displaced with respect to the strips of the other layer so that there are no rectilinear slits in the system. The time-of-flight system TOF provides a fast trigger to gamma-ray telescope readout electronics by measure the particles crossing time and position, and separates upward going particles from downward ones within 10^{-3} level. The TOF consists of hodoscope of four oriented perpendicularly layers of 1 cm thickness, 10 cm width, 100 cm (top) and 80 cm (bottom) length BC-408 plastic scintillation counters combined in two detector planes S1 and S2 located at the distance of 50 cm between the convertor-tracker C and coordinate-sensitive total absorption calorimeter CC2. The CC2 is 80 cm x 80 cm, $\sim 16X_0$ thick in vertical and $\sim 43X_0$ in transverse direction calorimeter based on the set of 440 CsI(Tl) crystals to measure the incoming particles energy with resolution of $\sim 2\%$ for gamma-rays with $E_\gamma \geq 100$ GeV and separate e^\pm and photons from hadrons at $\sim 5 \cdot 10^{-5}$ level. The preshower CC1 consists of two CsI(Tl) planes with total thickness of $\sim 2X_0$, the coordinate detector CD with two layers of double (x, y) SciFi tracking detectors (identical to convertor-tracker ones without tungsten) and fast plastic scintillation detector S3. Below CC2 the leakage plastic detector S4 is mounted. Plastic detectors AC, LD, S1-S4 are included in fast trigger logic in the main (vertical) and lateral (transverse) gamma-ray telescope apertures. The construction and front-end electronics units FEU of all detectors are similar with the exception of absence of temporal analysis circuits in AC_{lat} , LD, S3 and S4, and difference in counters number, length and orientation. Each side of AC_{top} , S1-S4 and only one side of AC_{lat} and LD is viewed by photo sensor modules on the basis of matrix of silicon photomultipliers (SiPM) mounted on printed circuit boards.

The gamma-ray telescope's anticoincidence detector system is a complex of segmented two-layer scintillation counters based on polyvinyltoluene BC-408, with separate events registration in each segment by means of SiPM matrices. The top and lateral anticoincidence detectors AC_{top} and $AC_{lat}1-4$ form protection for the main aperture of the gamma-ray telescope (vertical direction), while detectors C3, C4 and LD form protection for the lateral aperture of the

gamma-ray telescope (for particles falling onto the lateral surface of the CC2 calorimeter). A feature of the system is the use of a complex technique for compensating the «backsplash» effect caused by the impact on the anticoincidence system of low-energy secondary electrons and positrons resulting from the interactions of high-energy (> 5 GeV) gamma-rays with the gamma-ray telescope matter. In this case, erroneous blocking of «useful» events occurs, leading to a reduction of the detection efficiency. To compensate for this effect, the method of temporal analysis of the delay of the «backsplash» signal in the AC_{top} with respect to the signal from the time-of-flight system is used [4] in addition to segmentation of the detectors and making them multilayered. In this case, the segments of the corresponding detectors should have intrinsic time resolution of ~ 1 ns. More than 90% of “useful” events can be saved at the stage of fast hardware selection, using this technique according to preliminary estimates [5].

2. THE EXPERIMENTAL SETUP AND RESULTS OF MEASUREMENTS

The prototype of the anticoincidence detector system is an assembly of polyvinyltoluene BC-408 scintillation strip with dimensions of 1280 mm x 100 mm x 10 mm, wrapped with TYVEC reflection material and placed in 0.6 mm thick carbon fiber housings. The strip is viewed from two opposite ends by modules of photodetectors. The current version of the prototype uses matrices of six 6mm x 6mm SiPM mounted on a printed board with dimensions of 90 mm \times 11.5 mm. To improve the optical contact of SiPM with the scintillator surface the silicon grease BC-630 is used. Taking into account the need for obtaining both time and amplitude information from detectors, the SiPM type OnSemi MicroFC-60035-SMT-C1 having an additional «fast» output with a low capacitance are used, which allows simultaneously receive both a timing signal with a front of 2÷4 ns from the «fast» output, without additional analog signal shaping, and a signal with a front of ~ 200 ns from the «slow» output to measure the energy deposition in the detector segments. Signals from «fast» SiPM outputs are summed on a matrix of Schottky diodes type Skyworks SMS 7621-006LF, mounted on the same printed board as the SiPM (two diodes for each «fast» SiPM output to reduce the noise contribution from not

active SiPM in matrix [6]). The summed «fast» signal is additionally amplified by a factor of ~ 10 by an InGaP-based preamplifier type MMIC HMC589AST89ET mounted on a separate board, located at a distance of 5 mm from the SiPM board and connected to it through board-to-board connectors. The photodetector module is connected by cables of ~ 10 cm long to the FEU containing secondary power supplies and an additional signal amplification unit (~ 50 times) based on two AD8000 operational amplifiers. The signals from «slow» SiPM outputs are summed and fed into a preamplifier-shaper with pole-zero cancellation circuit based on two AD8000 operational amplifiers to form output analog signals with a rise time of ~ 3 ns and a width of ~ 10 ns placed in the same FEU.

The measurements were carried out on the beam of secondary positrons of the C-25P “PAKHRA” synchrotron [7] with an average energy of ~ 250 MeV, a FWHM of ~ 3 MeV and an average intensity of $\sim 10^3 \text{ cm}^{-2}\text{s}^{-1}$. The initial beam is limited by a lead collimator $\varnothing 15$ mm and 50 mm thick. To form the beam trigger signal (TRIG), a hodoscope [8] of three scintillation counters is used. To analyze temporal and amplitude information from the prototype, four-channel digital oscilloscope LeCroy WaveRunner 620Zi is applied. The measurement setup and scheme of the data acquisition in Fig. 2 are presented. The amplified «fast» or shaped «slow» analog signals from «left» and «right» ends of the prototype detector are split into two parts: one part is fed directly to the input of the oscilloscope for amplitude analysis, while the second one is fed to the input of the constant fraction discriminator (CFD) type ORTEC 935. The output CFD signal with duration of 20 ns goes to another input of the oscilloscope for temporal analysis, and also, through the delay lines type CAEN N108, to the inputs of double coincidence module LeCroy 622 for detection efficiency measurements. The coincidences of trigger signal with pulses from each end of the prototype, as well as with the logical sum (by OR) of signals from the ends, are registered. The trigger signal from the hodoscope is applied to the external synchronization input of the oscilloscope too. During the sessions, the amplitude and time resolution of the detector as a function of beam impact position relative to the detector center for

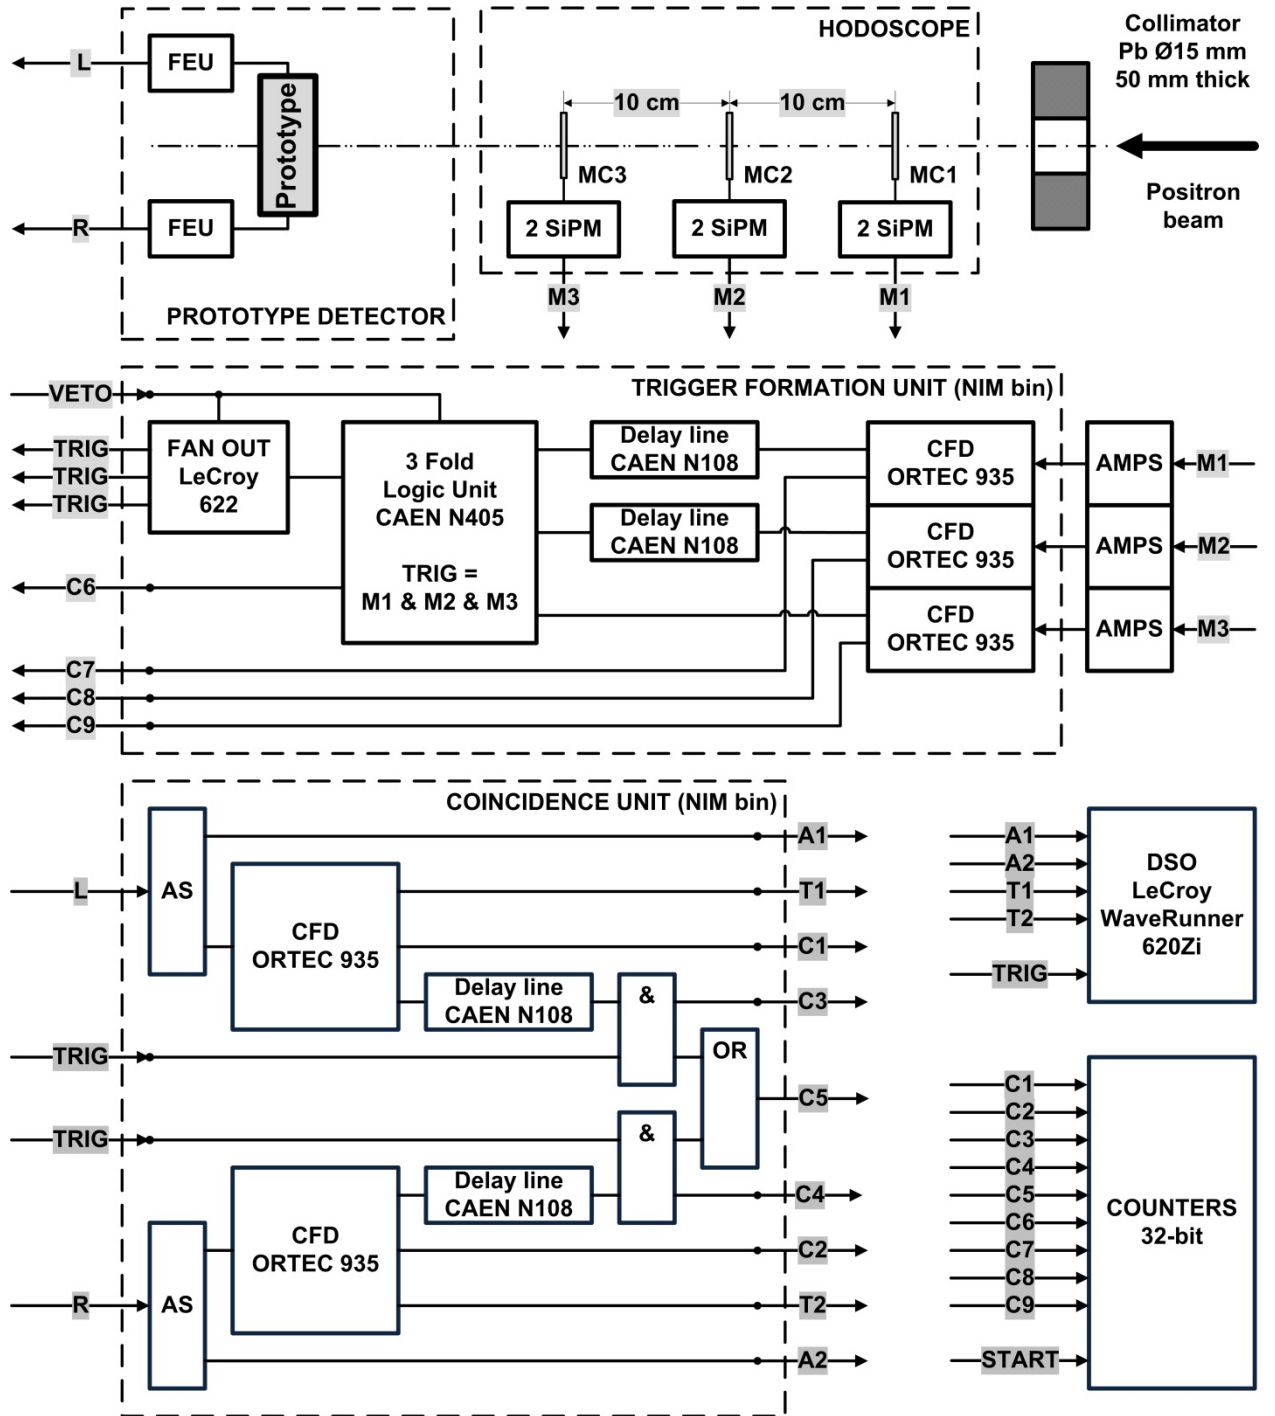


Fig. 2. Measurement setup and scheme of the data acquisition: FEU – front-end unit. L and R – analog signals from «left» and «right» ends of prototype detector respectively; A1÷A2 – signals for amplitude analysis; T1÷T2 – signals for temporal analysis; C1÷C9 – counting signals. VETO and START – logical external control signals from remote workstation; DSO – remotely operated digital oscilloscope LeCroy WaveRunner 620Zi. MC1÷MC3 - hodoscope of three 3x15x15 mm³ SC-301 polystyrene scintillation counters wrapped with MYLAR reflection material. The triple coincidence signal from hodoscope's counters (signals M1÷M3) forms the trigger signal TRIG with duration of 20 ns. The measured time resolution of the hodoscope is 104 ± 2 ps. AS – analog splitter; CFD – constant fraction discriminator type ORTEC 935; &, OR – AND, OR double coincidence logic type LeCroy 622; AMPS - preamplifier-shaper with pole-zero cancellation circuit.

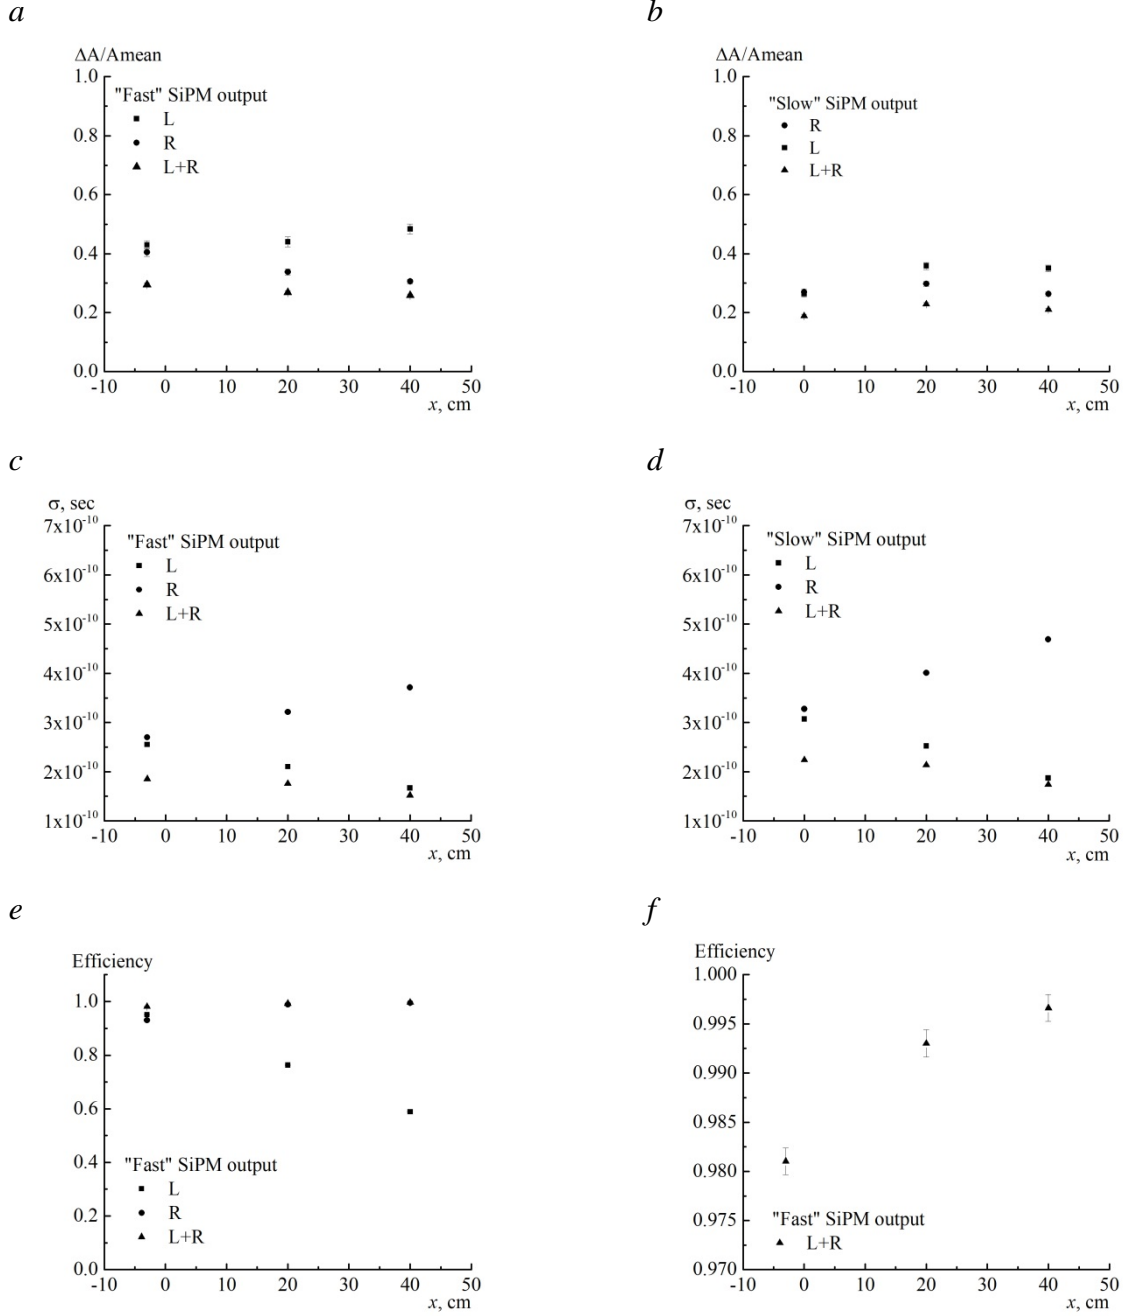


Fig. 3. The amplitude resolution (a, b), time resolution (c, d) and detection efficiency (e, f) of the prototype detector as a function of the beam impact position x relative to the detector center for «fast» (a, c, e, f) and «slow» (b, d) SiPM output, respectively. Fig. 2f shows the overall L+R efficiency from Fig. 2e on an enlarged scale. ΔA – FWHM of the amplitude distribution, A_{mean} – mean value of the amplitude. The designators L and R correspond to the «left» and «right» ends of the scintillator strip, respectively. L+R – combined resolution σ_{LR} at both ends obtained as $1/\sigma_{\text{LR}}^2 = 1/\sigma_{\text{L}}^2 + 1/\sigma_{\text{R}}^2$ for Figs. 2a-2d and logical sum (by OR) of signals from both strip ends for Figs. 2e-2f. Error bars are less than some points on the plots.

«fast» and shaped «slow» signals were studied. The charged particles detection efficiency was measured only for the «fast» SiPM output because of lack of accelerator time in this session. All measurements were carried out for the detection threshold corresponding to ~ 0.5 MIP (Minimum

Ionizing Particles energy deposition) for energy deposition at the center of the detector strip. Statistics at each point was $\sim 10^6$ particles for measurements of the detection efficiency and $\sim 10^4$ for other. The main measured results in Fig. 3 are shown. The using of the «fast» signal gives a $\sim 20\%$ better time resolution then «slow» one with additional analog signal shaping (185 ± 1 ps for the «fast» SiPM output versus 224 ± 2 ps for «slow» one, for particles falling at the center of the detector) and $\sim 30\%$ worse amplitude resolution ($29 \pm 1\%$ versus $22 \pm 1\%$, respectively). The detection efficiency for the «fast» signal is as good as 0.981 ± 0.001 , which corresponds to the value of 0.9996 for a two-layer detector.

3. CONCLUSIONS

The work presents the main characteristics of the prototype of anticoincidence system of the space-based gamma-ray telescope GAMMA-400 with light readout at both ends of scintillation strip (BC-408, 1280 mm x 100 mm x 10 mm) by modules of photodetectors consisting of six SiPM type OnSemi MicroFC-60035-SMT-C1 using both «fast» and «slow» outputs of SiPM. The measurements were performed on the beam of secondary positrons of the C-25P «PAKHRA» synchrotron of Lebedev Physical Institute with an average energy of ~ 250 MeV. The using of «fast» output of SiPM gives the intrinsic time resolution of the prototype by $\sim 20\%$ better compared to one obtained with «slow» shaped SiPM output but the amplitude resolution is worse by $\sim 30\%$ at the same time. The approach with simultaneous utilization «fast» SiPM output for time measurements and «slow» SiPM outputs for amplitude measurements allows us to reach the optimal result. In this case the scheme of the front-end electronics of time analysis channel becomes simpler and this approach can simplify the development and tuning of the system consisting of hundreds identical channels. The reached values of time resolution (185 ± 1 ps for the «fast» SiPM output) and amplitude resolution ($22 \pm 1\%$ for the «slow» one) in conjunction with obtained value of detection efficiency (≥ 0.9996 for two-layer detector) shows that this approach is well suitable for using in anticoincidence detectors of space-based gamma-ray telescope.

REFERENCES

1. A. Galper, O. Adriani, R. Aptekar, et al., Bull. Russ. Acad. Sci. Phys., **77** (11), 1339 (2013).
2. A. Galper, N. Topchiev, Yu. Yurkin., Astron. Rep., **62**, 882 (2018).
3. A. Syrov, V. Smirnov, V. Sokolov, et al., Cosmonautics and Rocket Engineering., **3**, 58 (2015).
4. M. Kheymits, A. Galper, I. Arkhangelskaja, A. Arkhangelskiy, Yu. Gusakov, V. Zverev, V. Kadilin, V. Kaplin, A. Leonov, P. Naumov, M. Runtso, S. Suchkov, N. Topchiev and Yu. Yurkin, Instrum. Exp. Tech., **59** (4), 508 (2016).
5. A. Leonov, A. Galper, N. Topchiev et al., Phys. At. Nucl., **82** (6), 855 (2019).
6. Signal Driven Multiplexing of Silicon Photomultiplier Arrays. Semiconductor Components Industries. LLC (2015). Publication order number: AND9772/D. <http://www.onsemi.com/pub/Collateral/AND9772-D.PDF>. Accessed November 18, 2022.
7. V. Alekseev, V. Baskov, V. Dronov et al., J. of Phys.: Conf. Ser., **1390**, 012127 (2019).
8. A. Arkhangelskiy, A. Galper, I. Arkhangelskaja et al., J. of Phys.: Conf. Ser., **1390**, 012130 (2019).

FIGURE CAPTIONS

Fig. 1. The physical scheme of the GAMMA-400 gamma-ray telescope.

Fig. 2. Measurement setup and scheme of the data acquisition: AS – analog splitter; CFD – constant fraction discriminator type ORTEC 935; &, OR – AND, OR double coincidence logic type LeCroy 622 respectively; DSO – remotely operated digital oscilloscope LeCroy WaveRunner 620Zi; AMPS - preamplifier-shaper with pole-zero cancellation circuit; FEU – front-end unit; L and R – analog signals from «left» and «right» ends of prototype detector respectively; MC1÷MC3 - hodoscope of three 3x15x15 mm³ SC-301 polystyrene scintillation counters wrapped with MYLAR reflection material. The triple coincidence signal from hodoscope's counters (signals M1÷M3) forms the trigger signal TRIG with duration of 20 ns. The measured time resolution of the hodoscope is 104 ± 2 ps. L÷R - analog signals from «left» and «right» ends of the prototype detector, A1÷A2 – signals for amplitude analysis, T1÷T2 – signals for temporal analysis, C1÷C9 – counting signals. VETO and START – logical external control signals from remote workstation.

Fig. 3. The amplitude resolution (a, b), time resolution (c, d) and detection efficiency (e, f) of the prototype detector as a function of the beam impact position x relative to the detector center for «fast» (a, c, e, f) and «slow» (b, d) SiPM output, respectively. Fig. 2f shows the overall L+R efficiency from Fig. 2e on an enlarged scale. ΔA – FWHM of the amplitude distribution, A_{mean} – mean value of the amplitude. The designators L and R correspond to the «left» and «right» ends of the scintillator strip, respectively. L+R – combined resolution σ_{LR} at both ends obtained as $1/\sigma_{LR}^2 = 1/\sigma_L^2 + 1/\sigma_R^2$ for Figs. 2a-2d and logical sum (by OR) of signals from both strip ends for Figs. 2e-2f. Error bars are less than some points on the plots.